

FIG. 1A

FIG. 1B

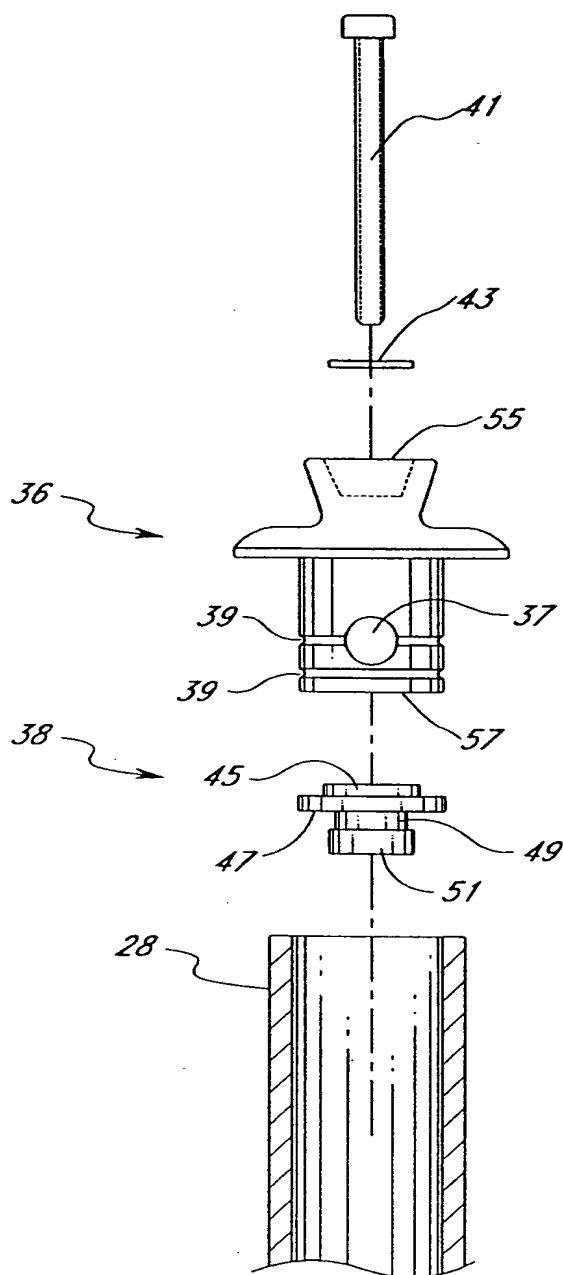
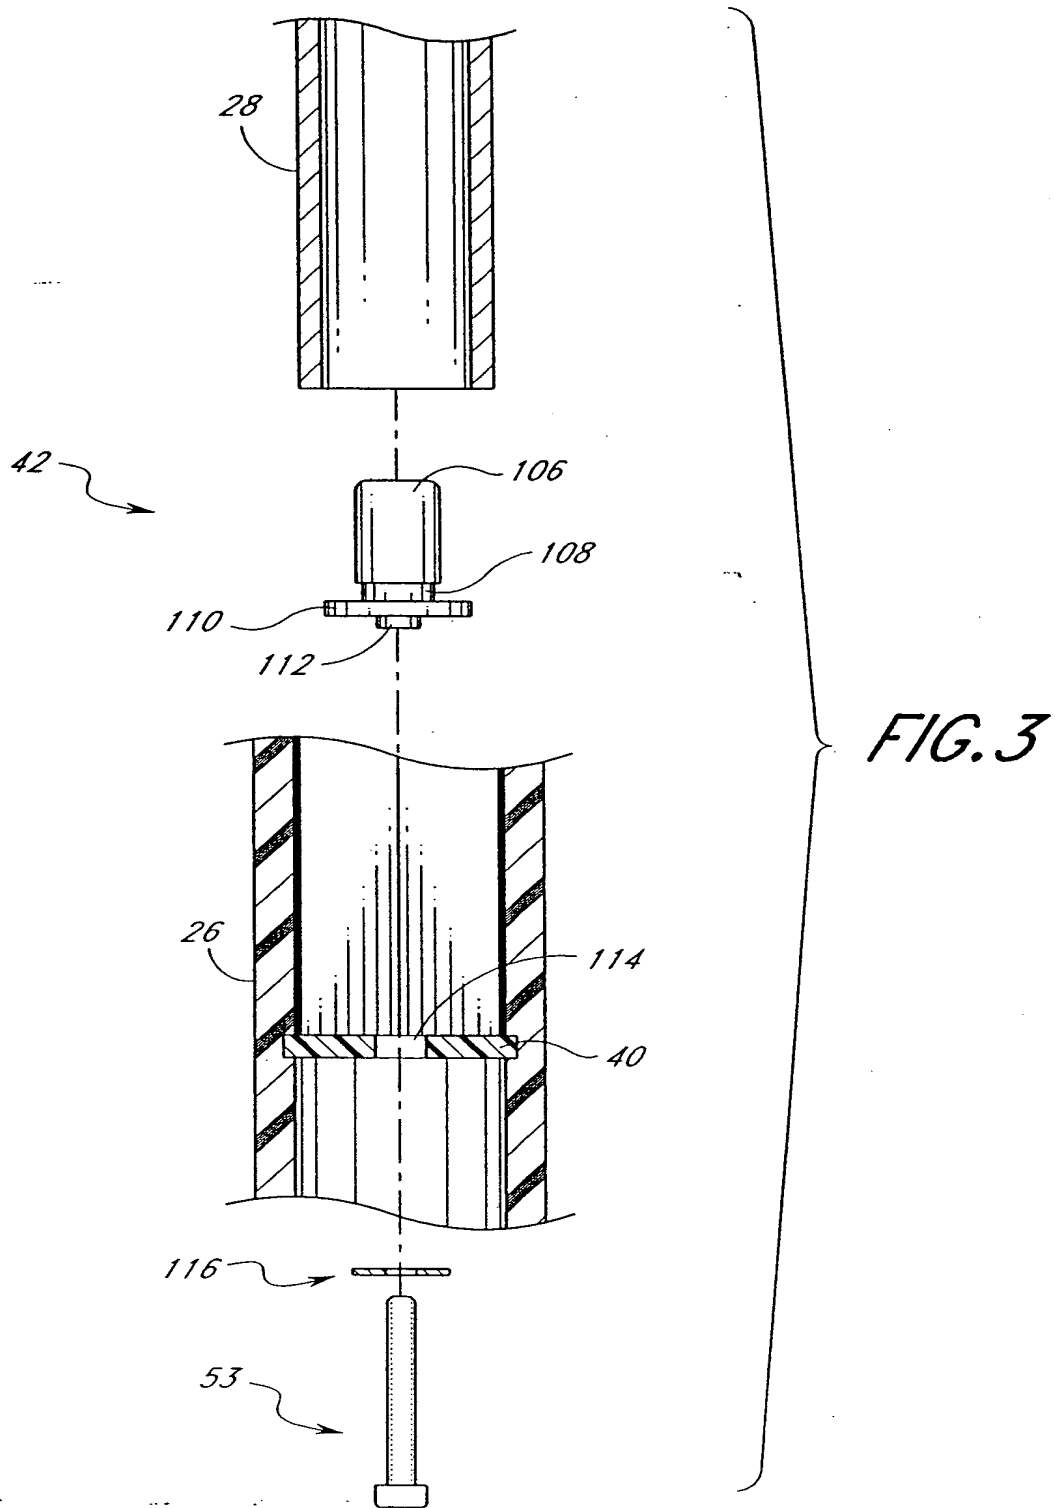


FIG. 2



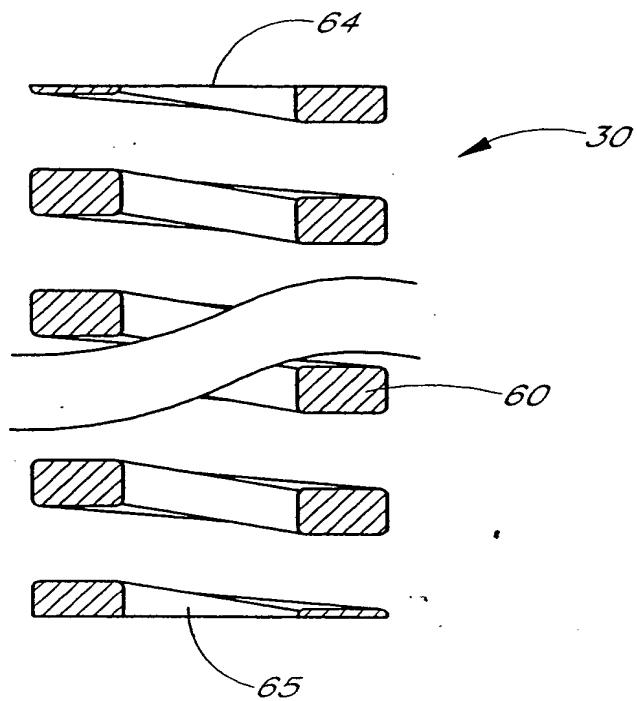


FIG. 4

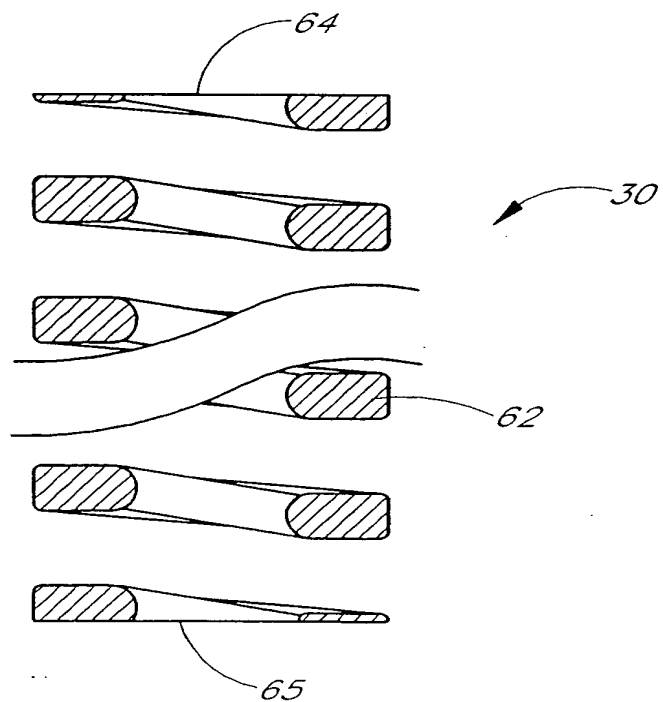


FIG. 5

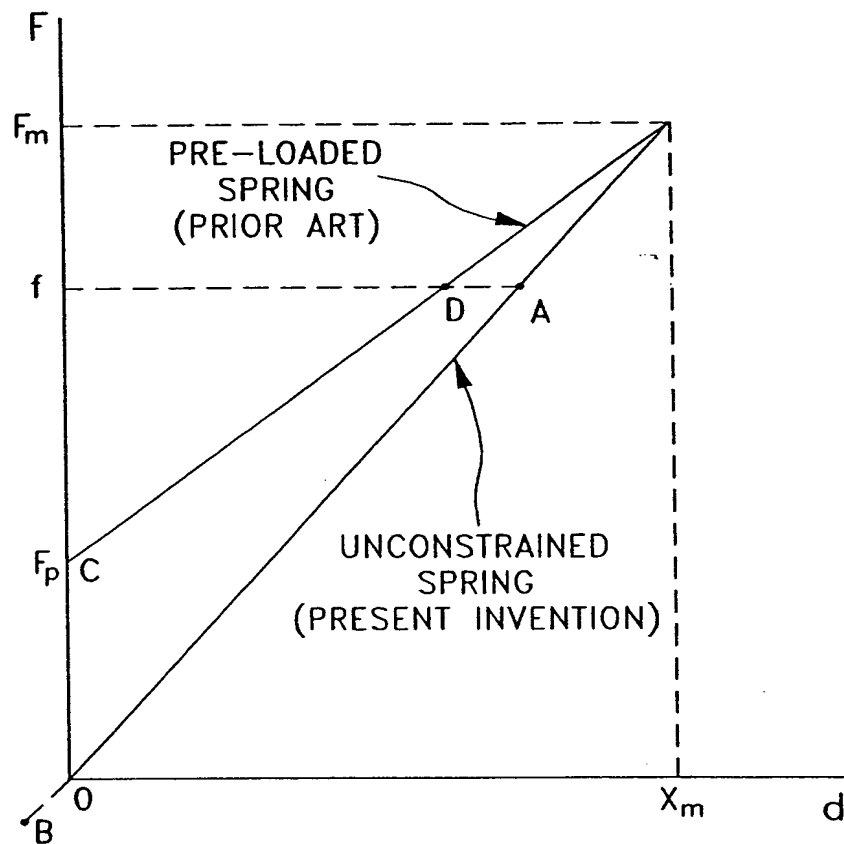


FIG. 6

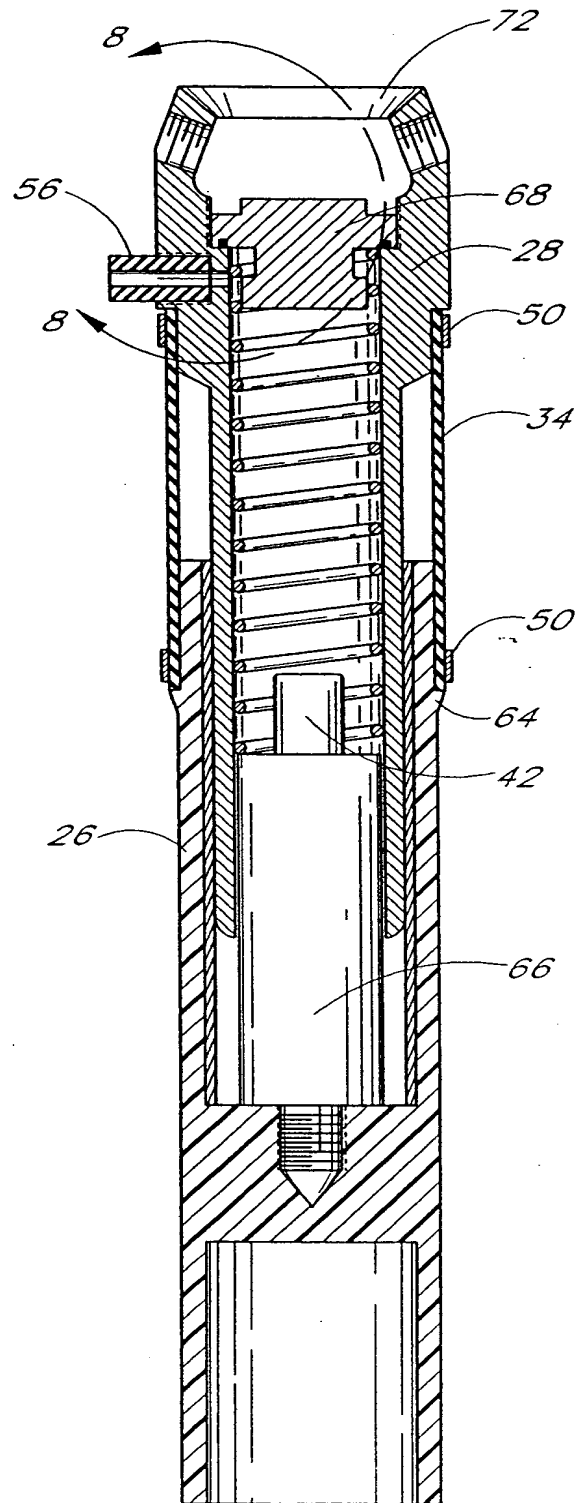


FIG. 7

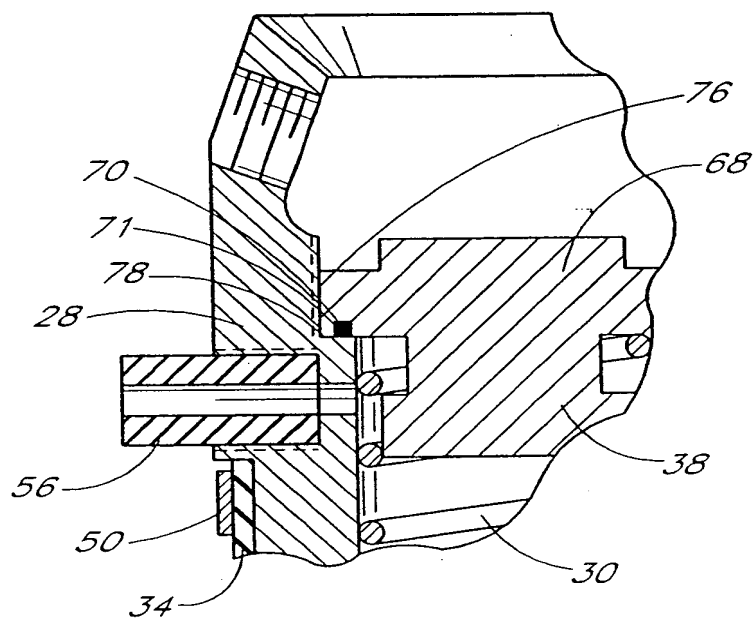


FIG. 8

SHOCK MODULE PROSTHESIS

Van L. Phillips et al.

Appl. No.: Unknown Atty Docket: FLEXFT.079C2

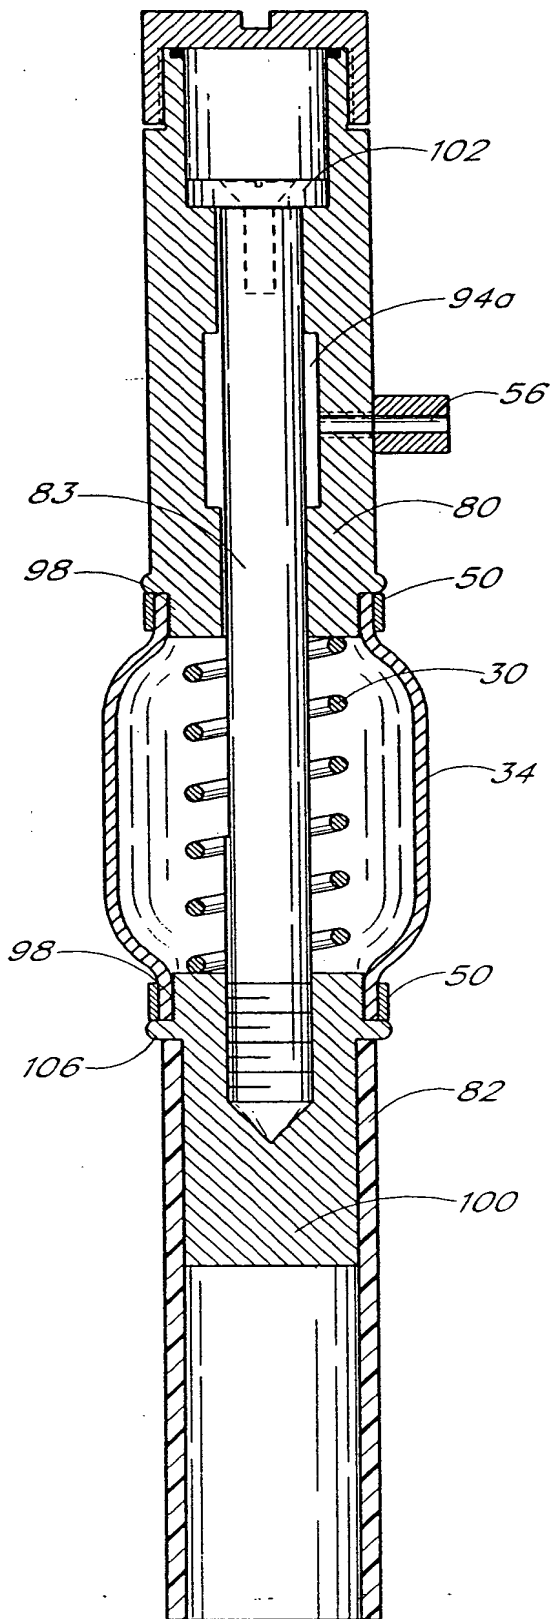


FIG. 9A

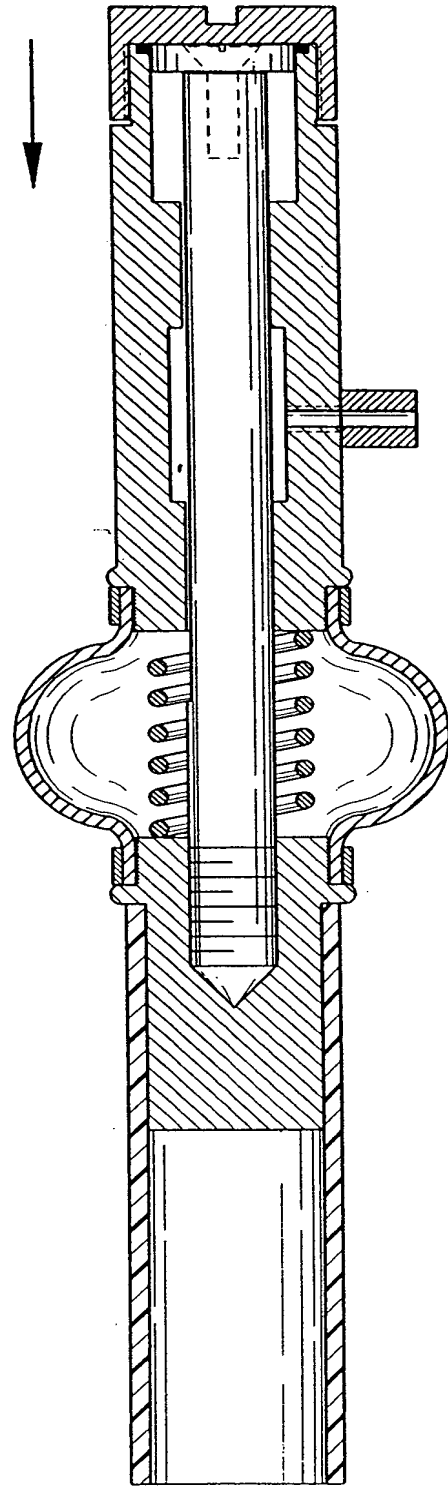


FIG. 9B



FIG. 10

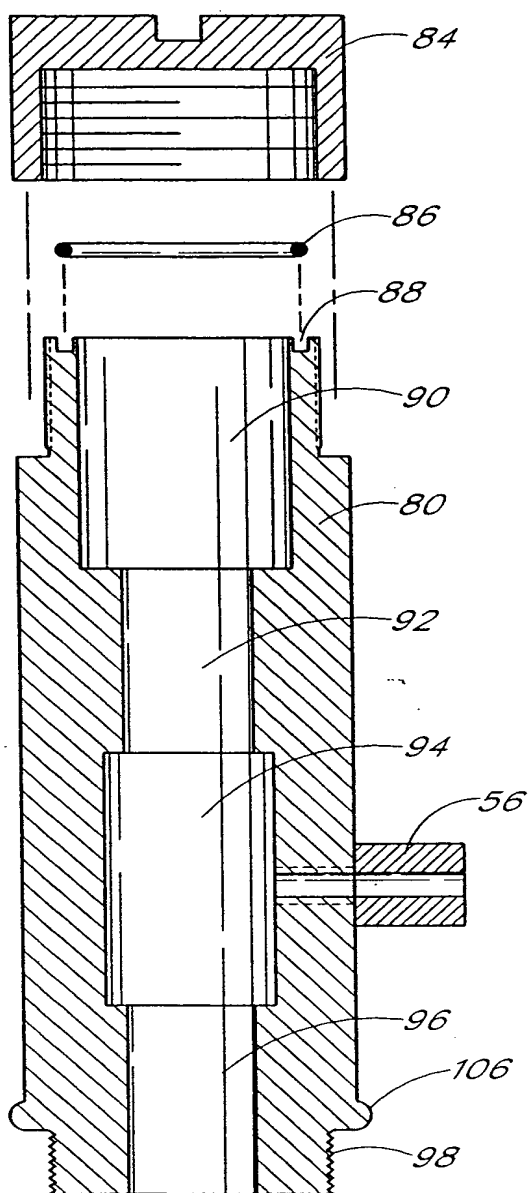


FIG. 11

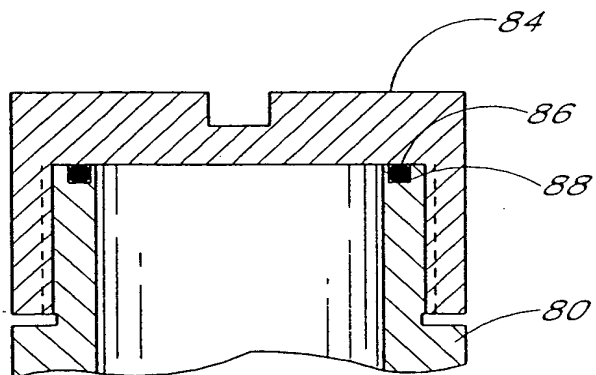


FIG. 12

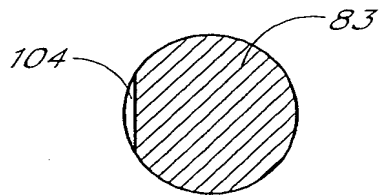
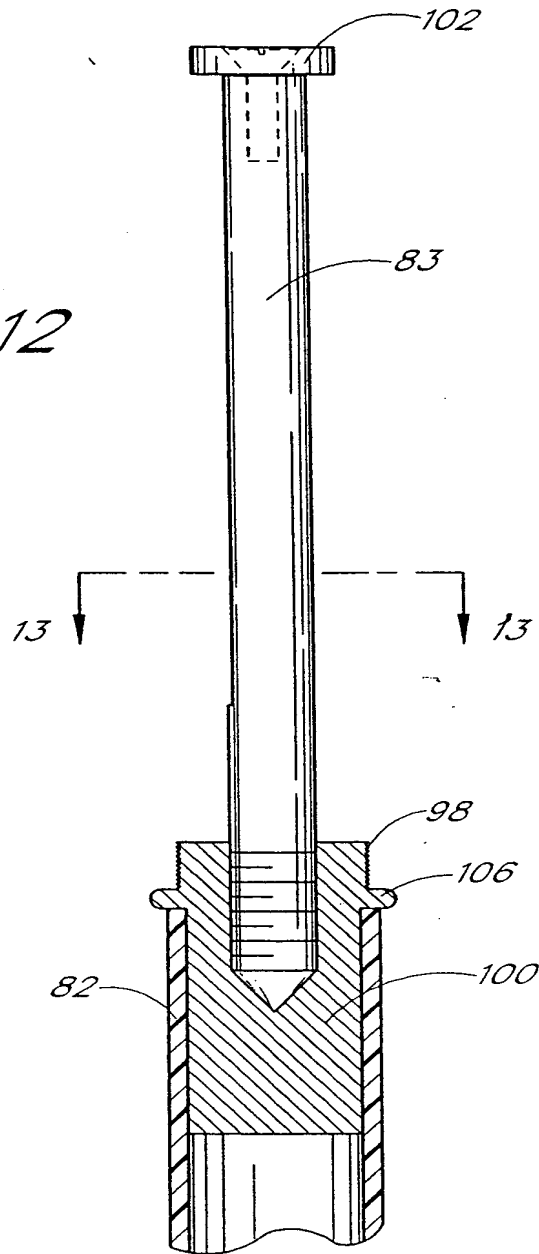


FIG. 13

FIG. 14

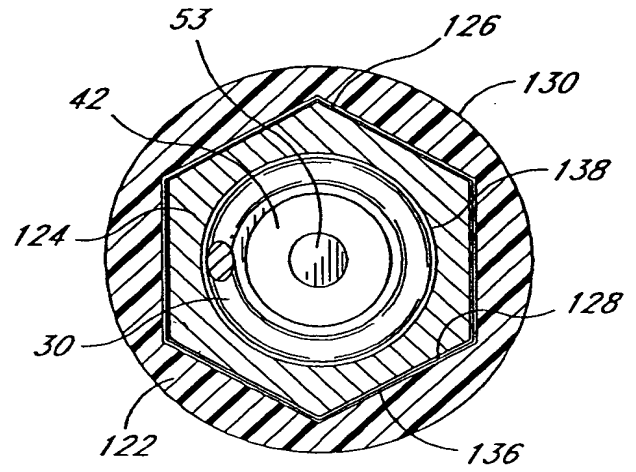
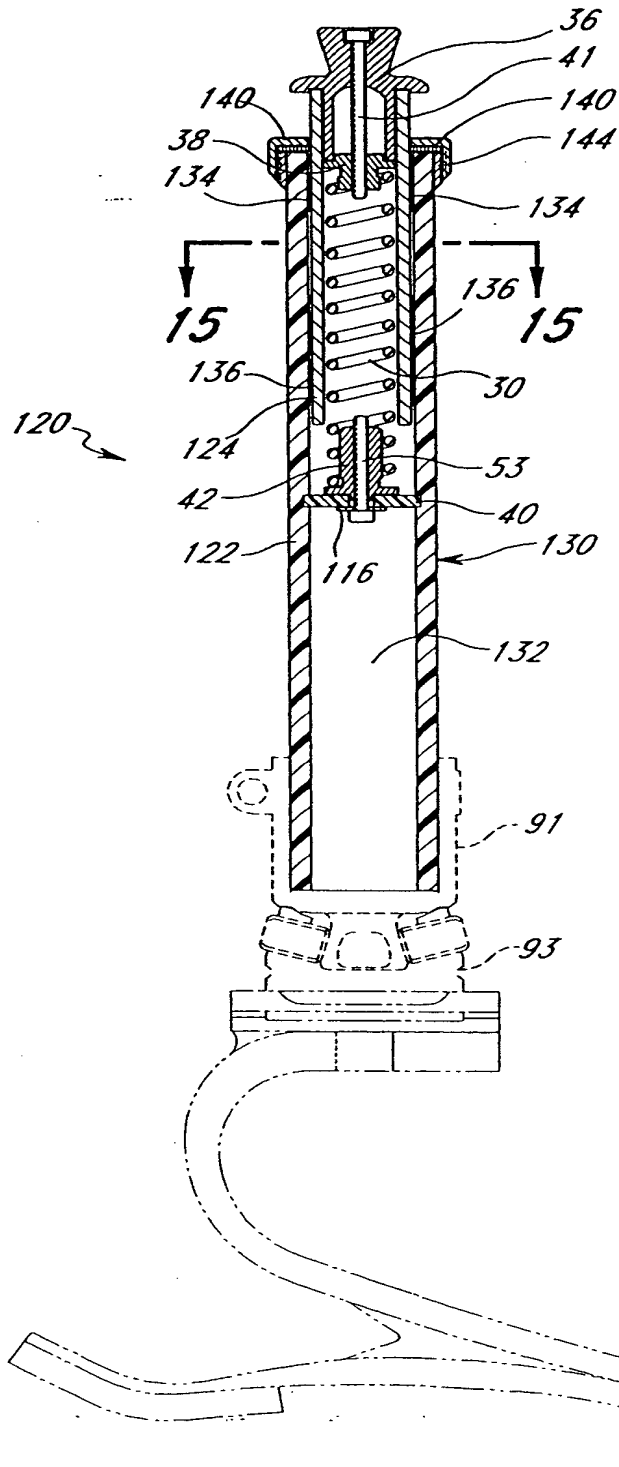


FIG. 15

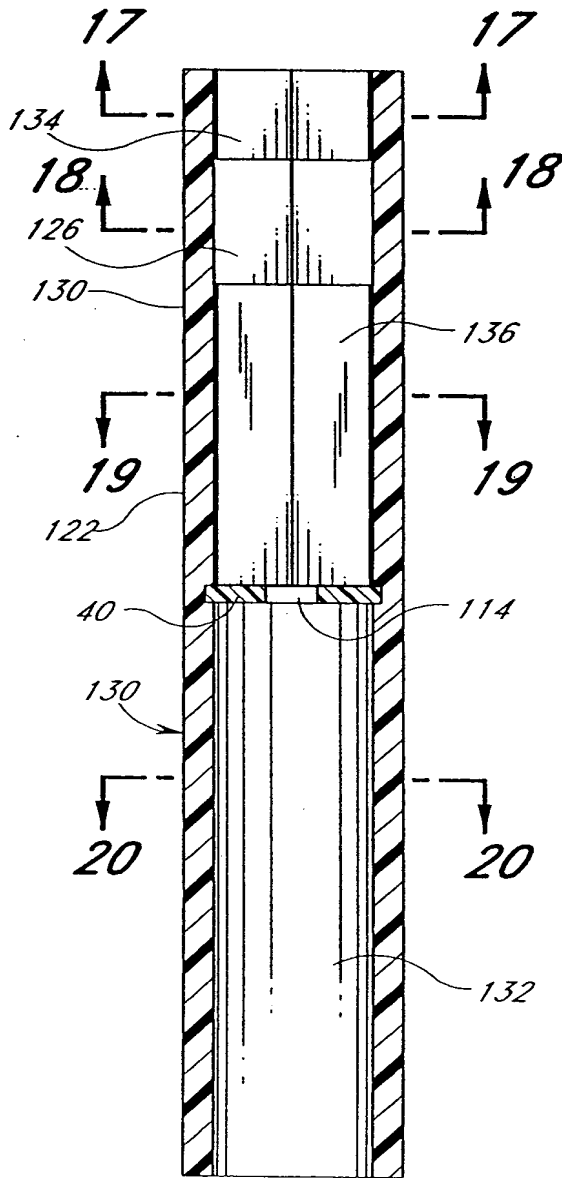


FIG. 16

